



Kansas City

tv_2-6.spa

Spectrum Analyzer

Trace Mode
Max Hold

Ref Lvl Offset
0.0 dB

Input Atten
0.0 dB

RBW
100 kHz


VBW
30 kHz

Detection
Peak

Trace Count
--

Reference Source
Int Std Accy

Sweep Time
348 ms

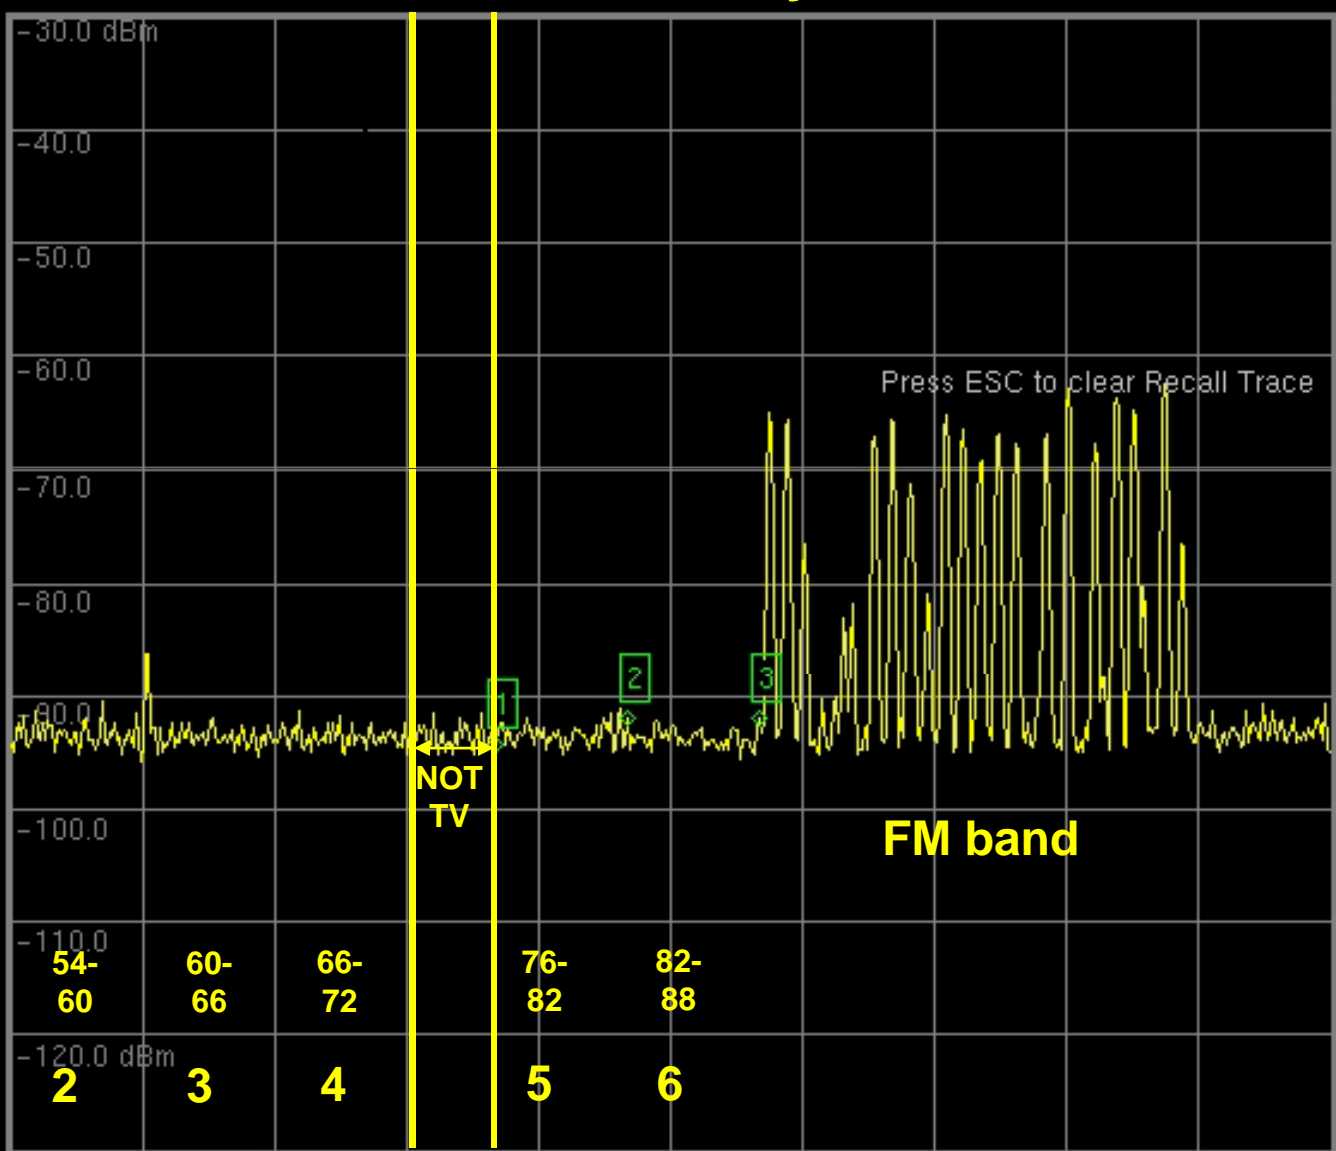

Start Freq 54.000 MHz

Stop Freq 114.000 MHz

Save

abc

def

ghi

jkl

mno

pqr

stu

vwx

yz - _

Back Space

Change

Save

Location

Change Type

Setup/JPG/...

Freq	Amplitude	Span	BW	Marker
------	-----------	------	----	--------

54-60	60-66	66-72	76-82	82-88
2	3	4	5	6



Kansas City

Trace A
Spectrum Analyzer

Trace Mode
Max Hold

Ref Lvl Offset
0.0 dB

Input Atten
0.0 dB

RBW
100 kHz


VBW
30 kHz

Detection
Peak

Trace Count
--

Reference Source
Int Std Accy

Sweep Time
348 ms

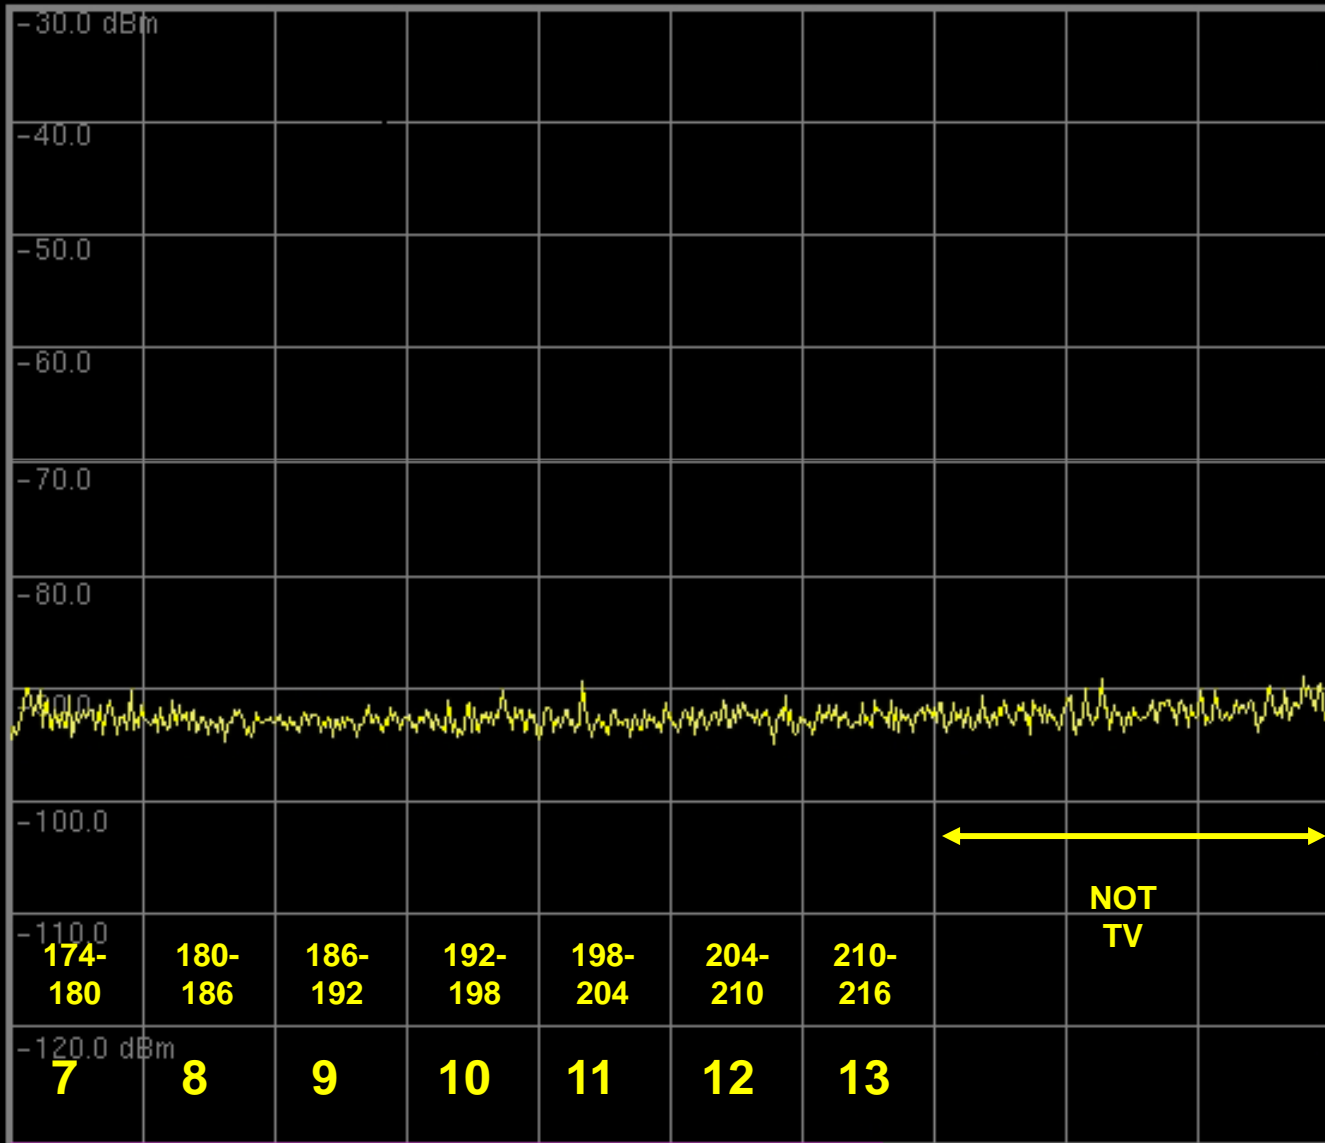

Center Freq 204.000 MHz

Span 60.000 MHz

Save

a b c

d e f

g h i

j k l

m n o

p q r

s t u

v w x

y z - _

Back Space

Change Save Location

Change Type

Setup/JPG/...

Freq	Amplitude	Span	BW	Marker
------	-----------	------	----	--------



Lectro Block 470 Kansas City

Trace A
Spectrum Analyzer

Trace Mode
Max Hold

Ref Lvl Offset
0.0 dB

Input Atten
0.0 dB

RBW
100 kHz


VBW
30 kHz

Detection
Peak

Trace Count
--

Reference Source
Int Std Accy

Sweep Time
348 ms

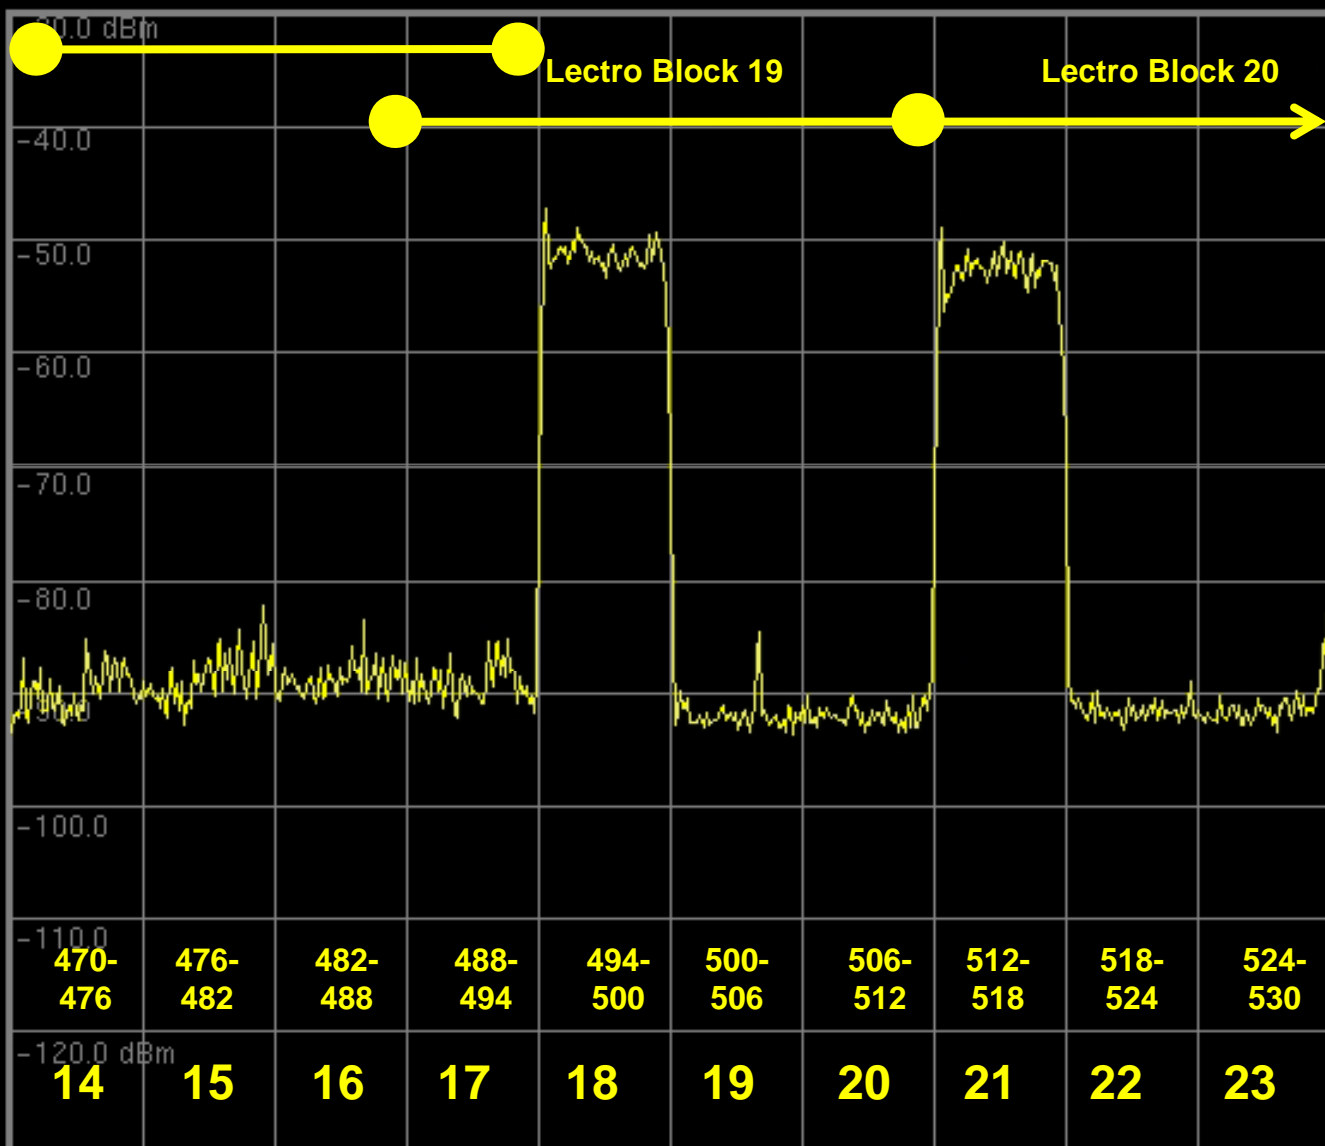

Center Freq 500.000 MHz

Span 60.000 MHz

Save

a b c

d e f

g h i

j k l

m n o

p q r

s t u

v w x

y z - _

Back Space

Change Save Location

Change Type

Setup/JPG/...

Freq	Amplitude	Span	BW	Marker
------	-----------	------	----	--------



Kansas City

Trace A
Spectrum Analyzer

Trace Mode
Max Hold

Ref Lvl Offset
0.0 dB

Input Atten
0.0 dB

RBW
100 kHz


VBW
30 kHz

Detection
Peak

Trace Count
--

Reference Source
Int Std Accy

Sweep Time
348 ms

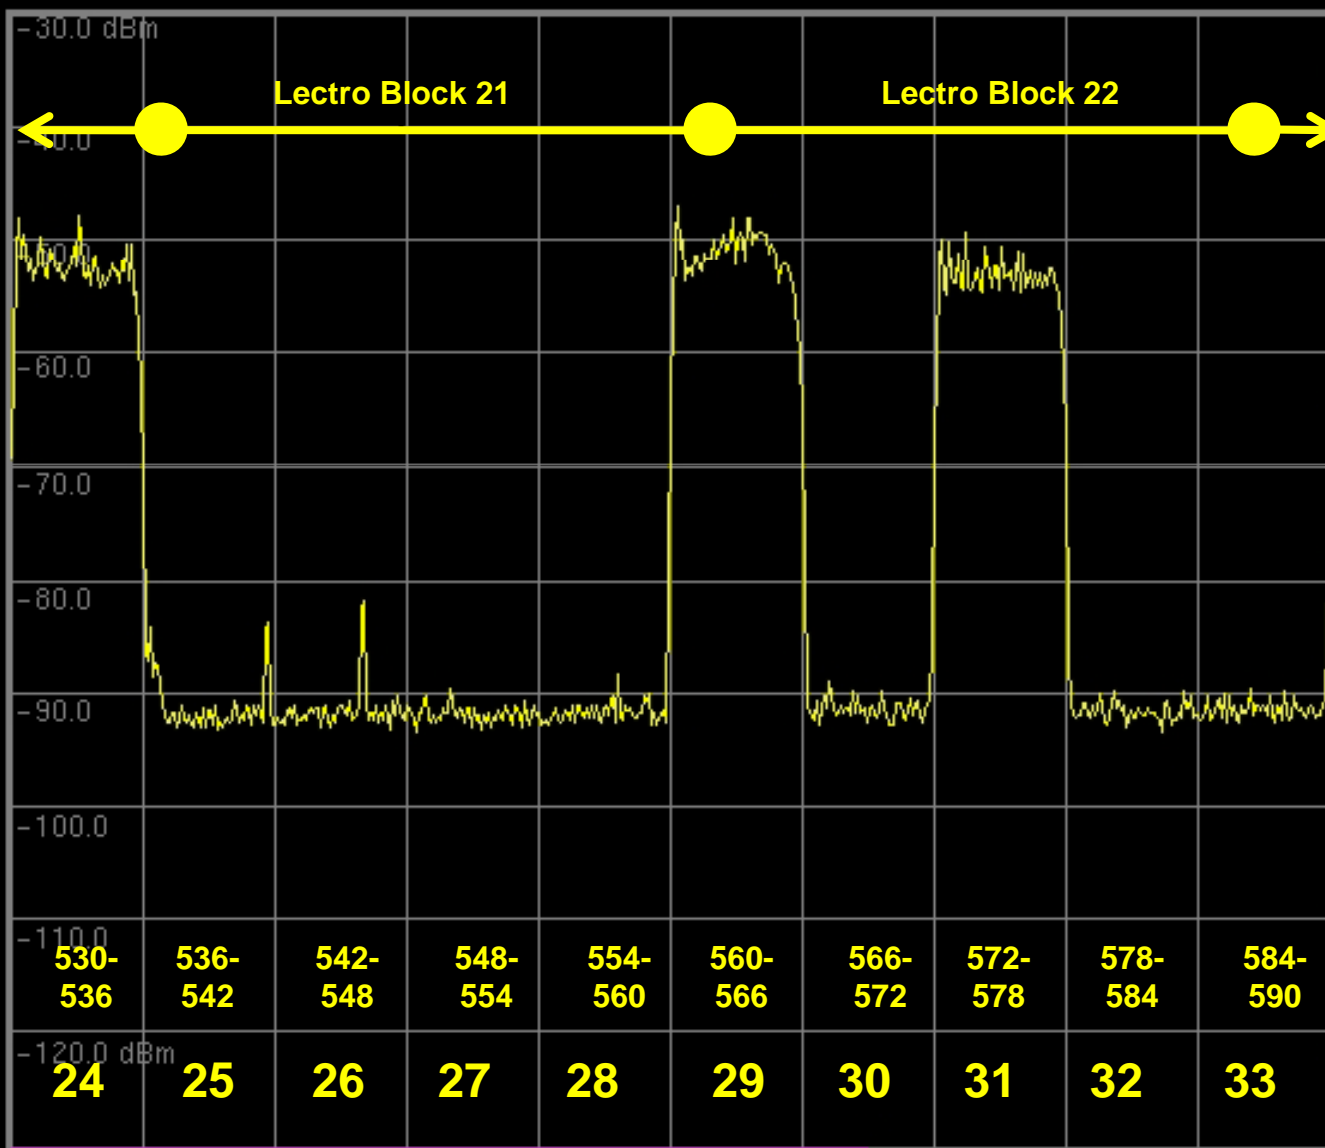

Center Freq 560.000 MHz

Span 60.000 MHz

Save

abc

def

ghi

jkl

mno

pqr

stu

vwx

yz - _

Back Space

Change Save Location

Change Type

Setup/JPG/...

Freq	Amplitude	Span	BW	Marker
------	-----------	------	----	--------



Kansas City

Trace A
Spectrum Analyzer

Trace Mode
Max Hold

Ref Lvl Offset
0.0 dB

Input Atten
0.0 dB

RBW
100 kHz


VBW
30 kHz

Detection
Peak

Trace Count
--

Reference Source
Int Std Accy

Sweep Time
348 ms

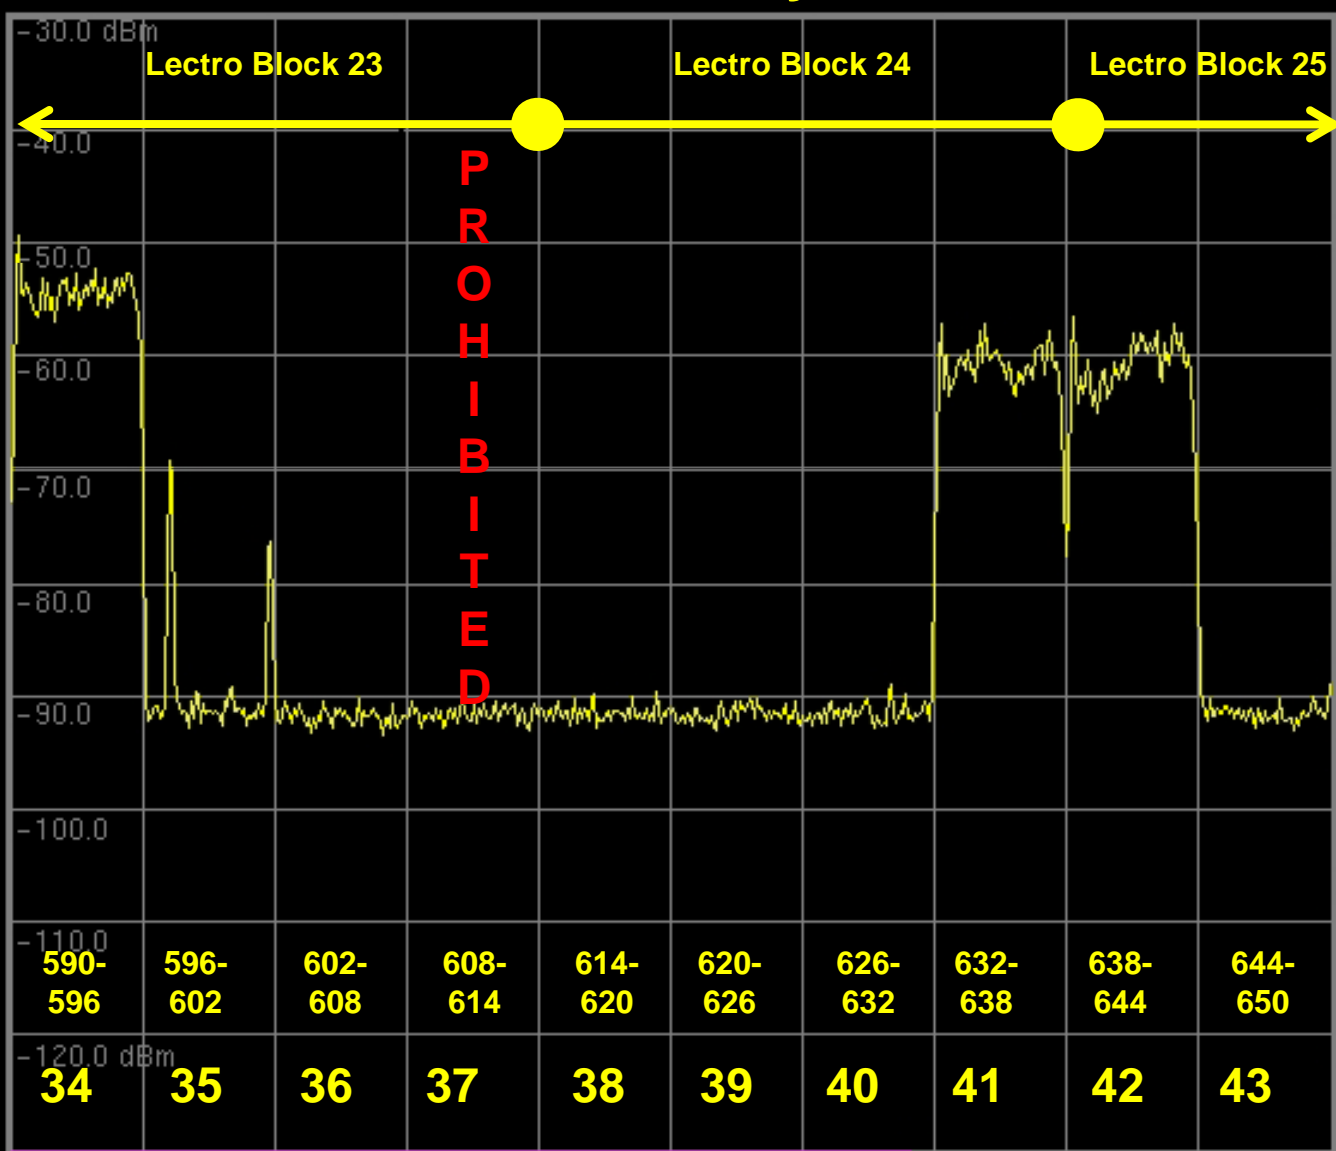

Center Freq 620.000 MHz **ASTRO** Span 60.000 MHz

- Save
- abc
- def
- ghi
- jkl
- mno
- pqr
- stu
- vwx
- yz - _
- Back Space
- Change Save Location
- Change Type
- Setup/JPG/...

Freq	Amplitude	Span	BW	Marker
------	-----------	------	----	--------



Kansas City

Trace A
Spectrum Analyzer

Trace Mode
Max Hold

Ref Lvl Offset
0.0 dB

Input Atten
0.0 dB

RBW
100 kHz


VBW
30 kHz

Detection
Peak

Trace Count
--

Reference Source
Int Std Accy

Sweep Time
348 ms

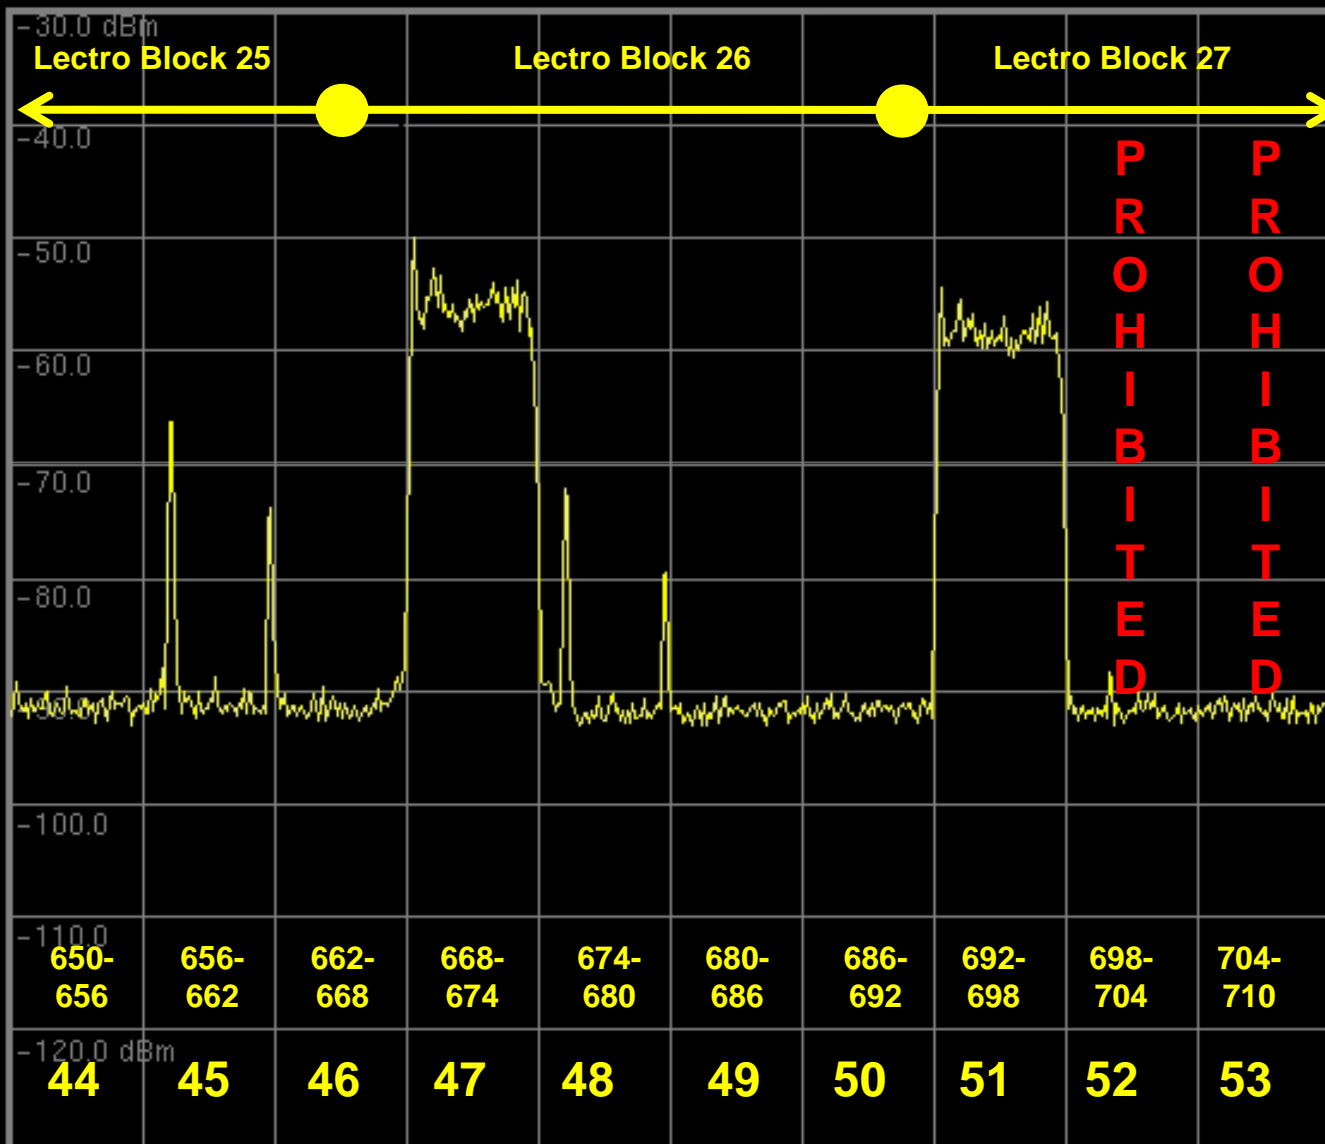

Center Freq 680.000 MHz

Span 60.000 MHz

Save

a b c

d e f

g h i

j k l

m n o

p q r

s t u

v w x

y z - _

Back Space

Change

Save

Location

Change Type

Setup/JPG/...

Freq

Amplitude

Span

BW

Marker



Kansas City

Trace A
Spectrum Analyzer

Trace Mode
Max Hold

Ref Lvl Offset
0.0 dB

Input Atten
0.0 dB

RBW
100 kHz


VBW
30 kHz

Detection
Peak

Trace Count
--

Reference Source
Int Std Accy

Sweep Time
348 ms

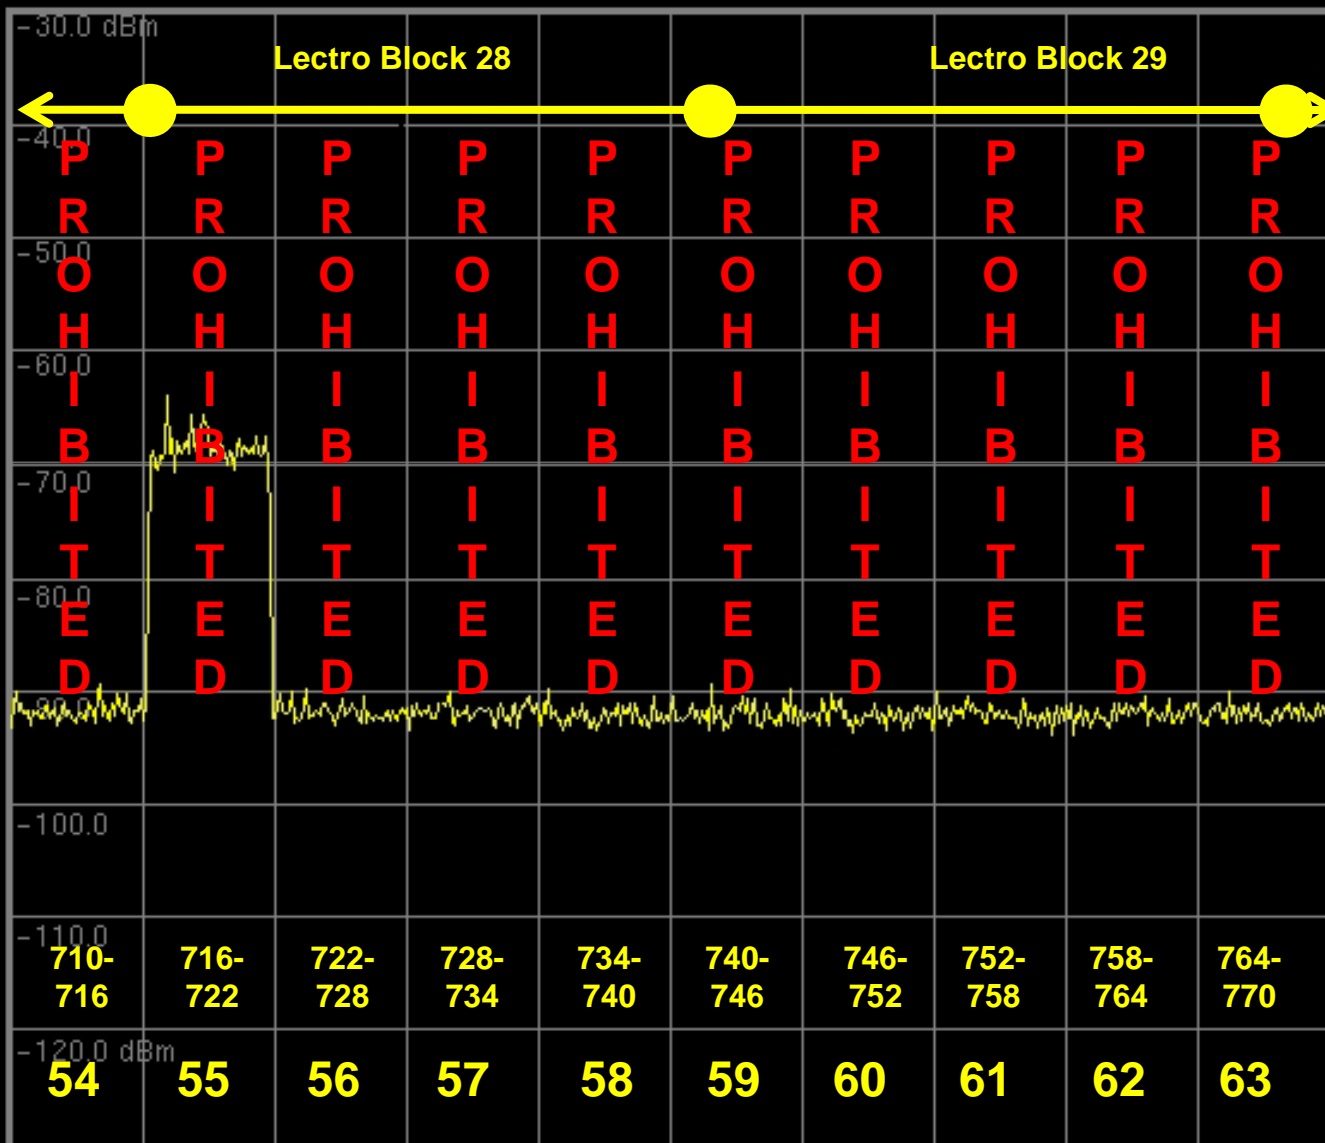

Center Freq 740.000 MHz

Span 60.000 MHz

Save

abc

def

ghi

jkl

mno

pqr

stu

vwx

yz - _

Back Space

Change Save Location

Change Type

Setup/JPG/...

Freq	Amplitude	Span	BW	Marker
------	-----------	------	----	--------



Kansas City

Trace A
Spectrum Analyzer

Trace Mode
Max Hold

Ref Lvl Offset
0.0 dB

Input Atten
0.0 dB

RBW
100 kHz


VBW
30 kHz

Detection
Peak

Trace Count
--

Reference Source
Int Std Accy

Sweep Time
348 ms

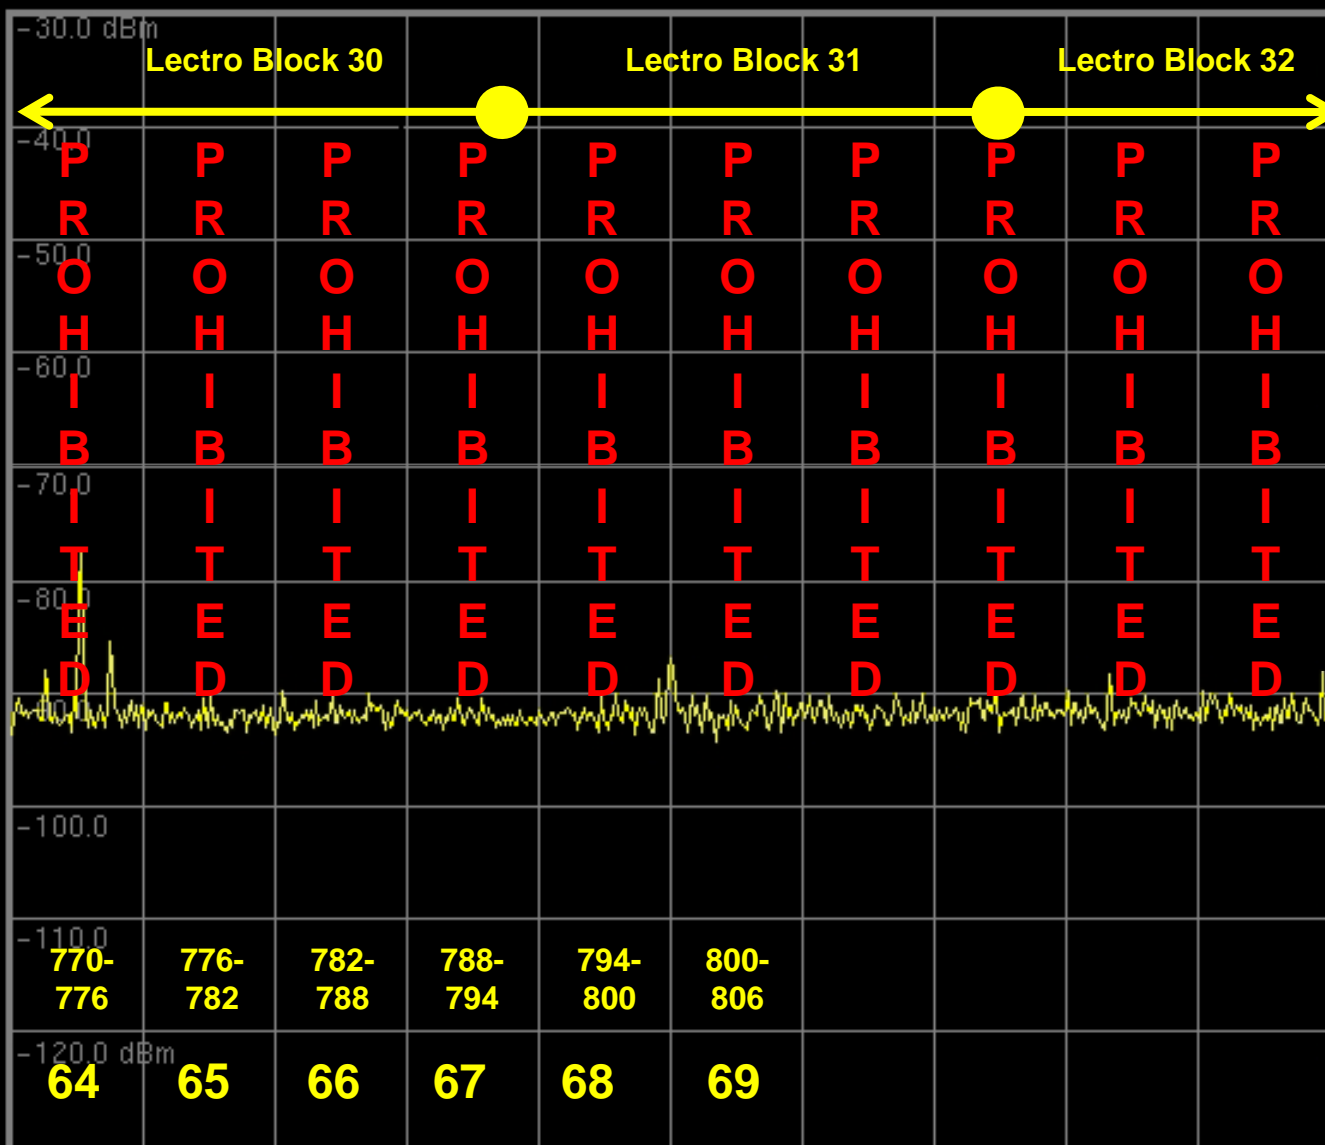

Center Freq 800.000 MHz

Span 60.000 MHz

Save

a b c

d e f

g h i

j k l

m n o

p q r

s t u

v w x

y z - _

Back Space

Change

Save

Location

Change Type

Setup/JPG/...

Freq

Amplitude

Span

BW

Marker